ASSMANN Distribution Sp. z o.o.
ul. Szczecińska 19, 54-517 Wrocław
NIP: 8951883569 / REGON: 020543570
+48 71 326 71 40 +48 71 326 71 41
office@assmann.pl / www.assmann.pl

ASSMANN

INFORMACJE NA TEMAT FABRYCZNEGO CERTYFIKATU KALIBRACJI MIERNIKA FIRMY

FLUKE networks™

Firma ASSMANN Distribution Sp. z o.o., jako autoryzowany dystrybutor produktów marki FLUKE Networks, informuje, że każdy miernik schodzący z taśmy produkcyjnej otrzymuje fabryczny certyfikat kalibracji. Natomiast zgodnie z tym dokumentem (opisywany fragment zaznaczony w ZAŁĄCZNIK NR 1 / zdj. 1a i 1b), jako początek 12 miesięcznego cyklu kalibracji uznaje się moment wykonania pierwszego pomiaru, o ile urządzenie przed tym było przechowywane przez sześć miesięcy lub krócej.

.....

Konrad Żaczek
Product manager

ASSMANN Distribution Sp. z o.o.
ul. Szczecińska 19, 54-517 Wrocław
NIP: 8951883569 / REGON: 020543570
+48 71 326 71 40 +48 71 326 71 41
office@assmann.pl / www.assmann.pl

ASSMANN

ZAŁĄCZNIK NR 1

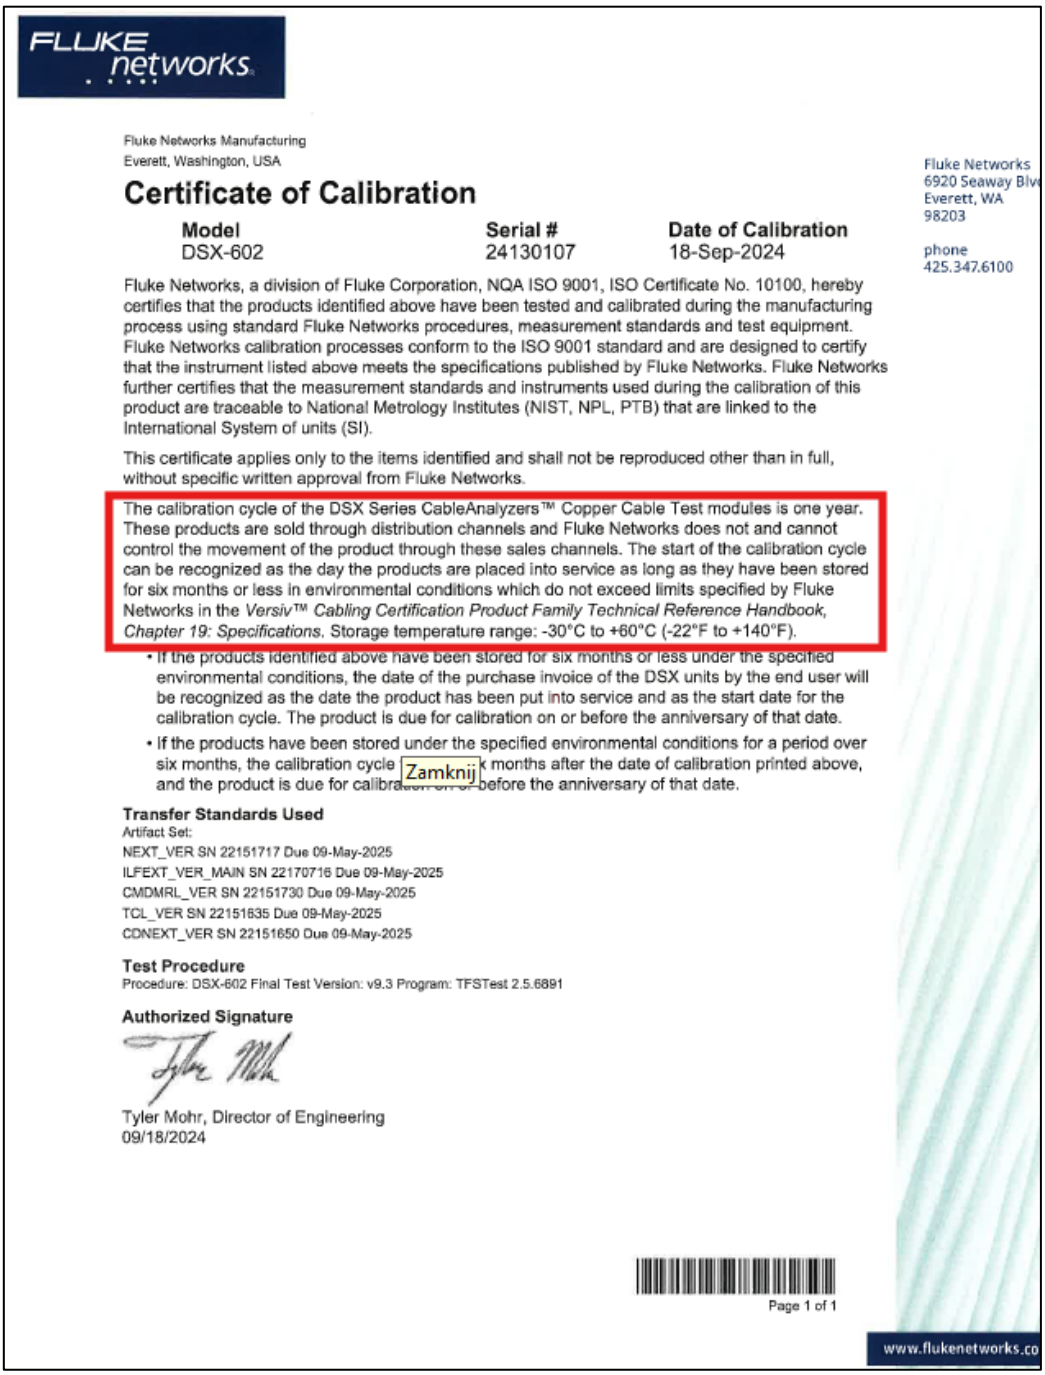

FLUKE networks

Fluke Networks Manufacturing
Everett, Washington, USA

Certificate of Calibration

Model	Serial #	Date of Calibration
DSX-602	24130107	18-Sep-2024

Fluke Networks
6920 Seaway Blv
Everett, WA
98203

phone
425.347.6100

Fluke Networks, a division of Fluke Corporation, NQA ISO 9001, ISO Certificate No. 10100, hereby certifies that the products identified above have been tested and calibrated during the manufacturing process using standard Fluke Networks procedures, measurement standards and test equipment. Fluke Networks calibration processes conform to the ISO 9001 standard and are designed to certify that the instrument listed above meets the specifications published by Fluke Networks. Fluke Networks further certifies that the measurement standards and instruments used during the calibration of this product are traceable to National Metrology Institutes (NIST, NPL, PTB) that are linked to the International System of units (SI).

This certificate applies only to the items identified and shall not be reproduced other than in full, without specific written approval from Fluke Networks.

The calibration cycle of the DSX Series CableAnalyzers™ Copper Cable Test modules is one year. These products are sold through distribution channels and Fluke Networks does not and cannot control the movement of the product through these sales channels. The start of the calibration cycle can be recognized as the day the products are placed into service as long as they have been stored for six months or less in environmental conditions which do not exceed limits specified by Fluke Networks in the *Versiv™ Cabling Certification Product Family Technical Reference Handbook, Chapter 19: Specifications*. Storage temperature range: -30°C to +60°C (-22°F to +140°F).

- If the products identified above have been stored for six months or less under the specified environmental conditions, the date of the purchase invoice of the DSX units by the end user will be recognized as the date the product has been put into service and as the start date for the calibration cycle. The product is due for calibration on or before the anniversary of that date.
- If the products have been stored under the specified environmental conditions for a period over six months, the calibration cycle [Zamknij] months after the date of calibration printed above, and the product is due for calibration on or before the anniversary of that date.

Transfer Standards Used
Artifact Set:
NEXT_VER SN 22151717 Due 09-May-2025
ILFEXT_VER_MAIN SN 22170716 Due 09-May-2025
CMDMRL_VER SN 22151730 Due 09-May-2025
TCL_VER SN 22151635 Due 09-May-2025
CDNEXT_VER SN 22151650 Due 09-May-2025

Test Procedure
Procedure: DSX-602 Final Test Version: v9.3 Program: TFSTest 2.5.6891

Authorized Signature

Tyler Mohr, Director of Engineering
09/18/2024

Page 1 of 1

www.flukenetworks.co

Zdj.1a. Przykład fabrycznego certyfikatu kalibracji miernika firmy Fluke Networks.

ASSMANN Distribution Sp. z o.o.
ul. Szczecińska 19, 54-517 Wrocław
NIP: 8951883569 / REGON: 020543570
+48 71 326 71 40 +48 71 326 71 41
office@assmann.pl / www.assmann.pl

ASSMANN

ZAŁĄCZNIK NR 1

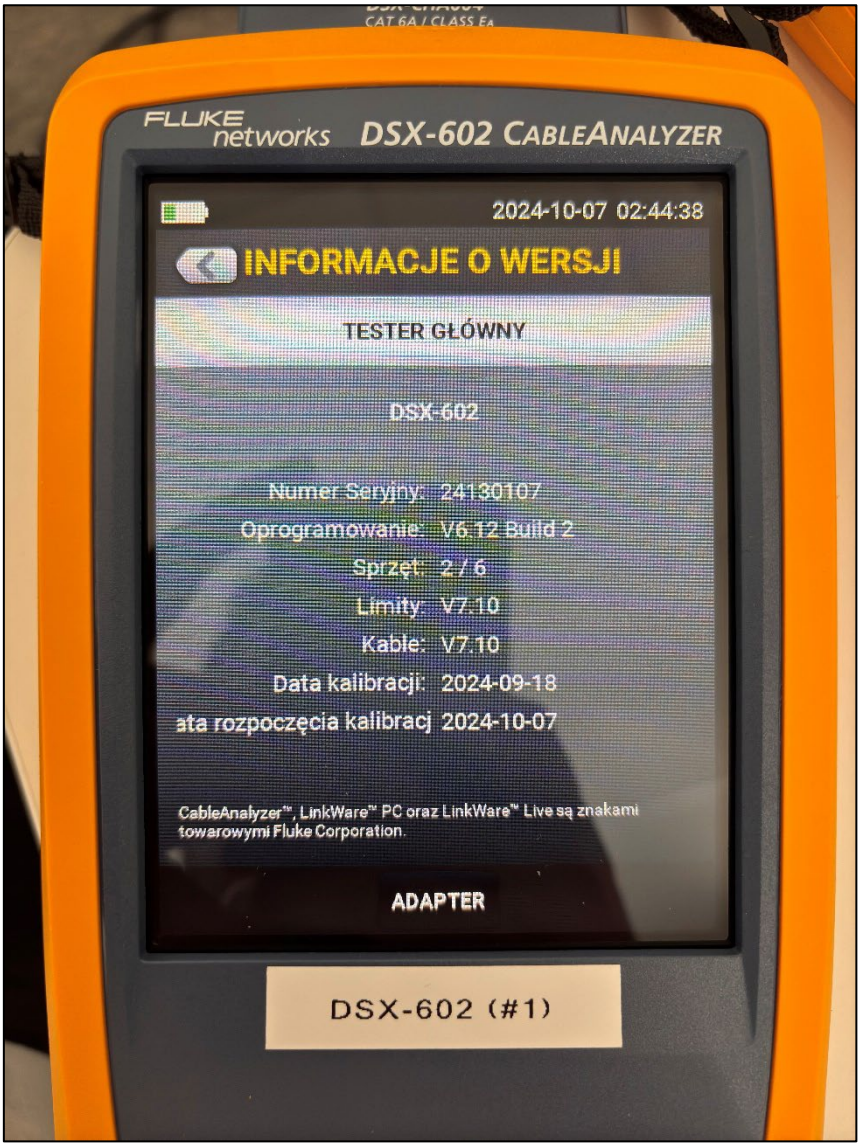

Zdj. 2. Zdjęcie ekranu miernika DSX-602, na którym zostały wyświetlone informacje dotyczące okresu kalibracji obu modułów pomiarowych DSX. Data wykonania kalibracji fabrycznej oraz data rozpoczęcia kalibracji – czyli dzień wykonania pierwszego pomiaru.